


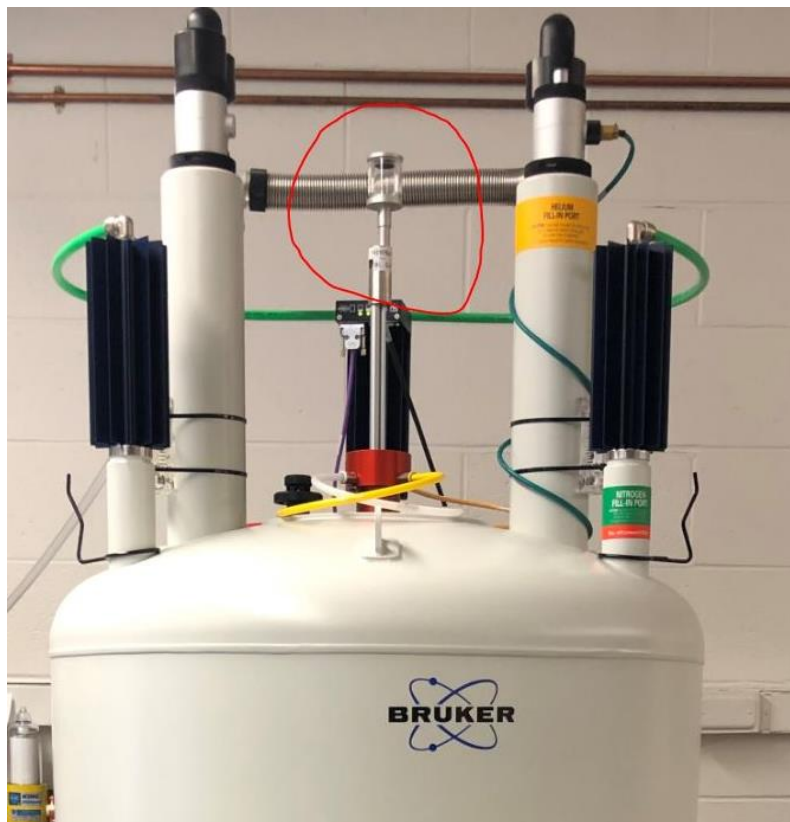


Sample holding chamber

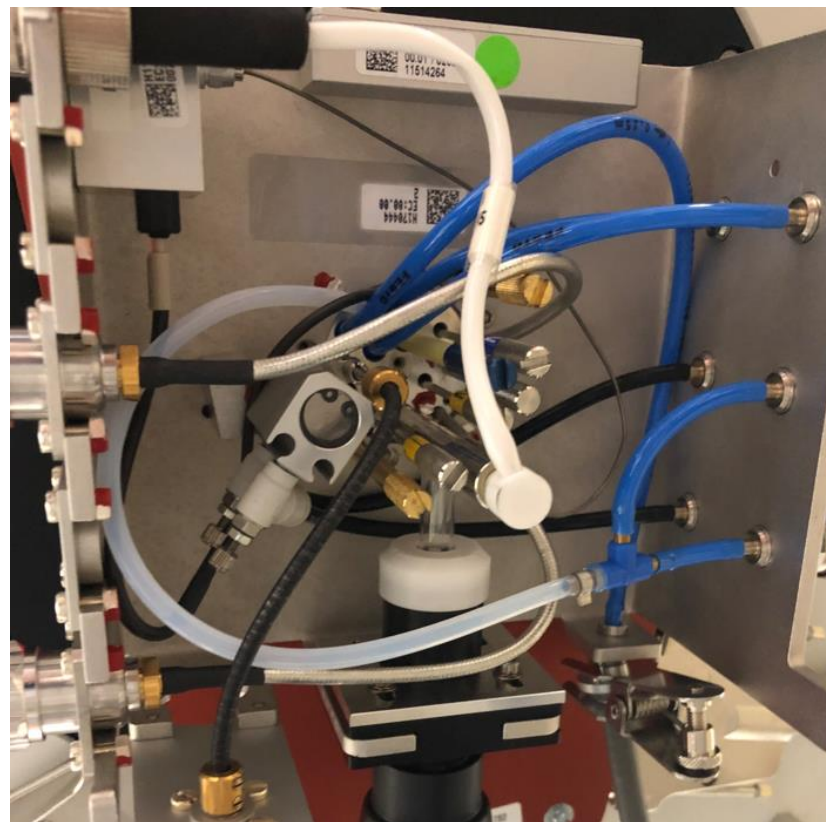

H-F/X DR probe bottom

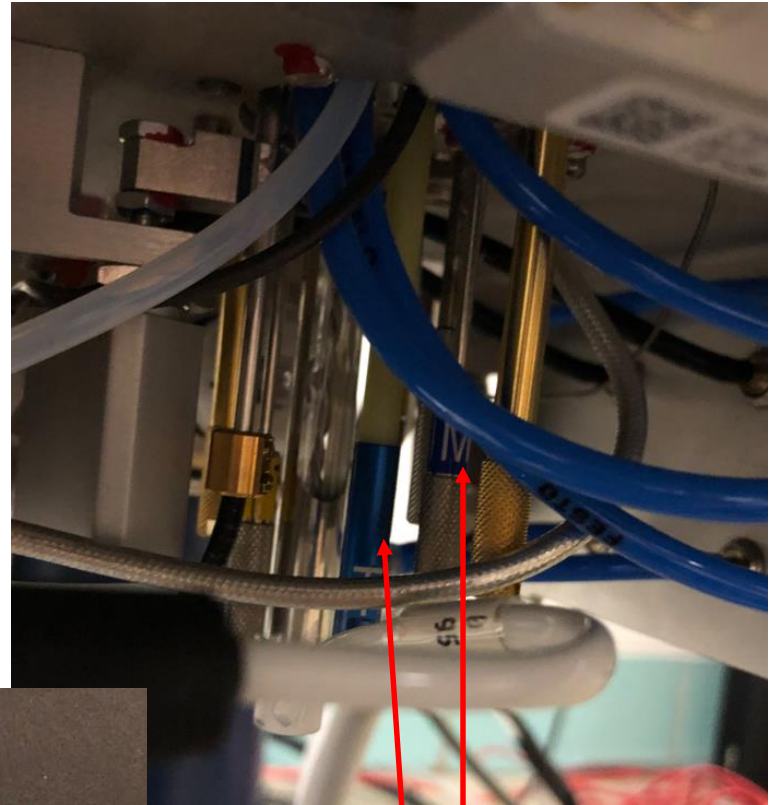

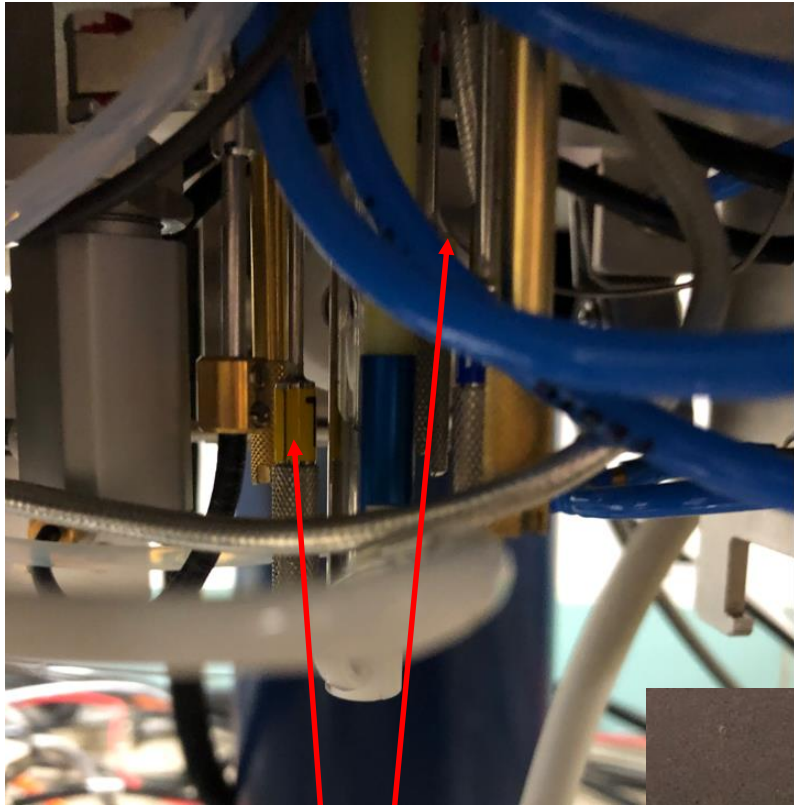

$^1\text{H}/^{19}\text{F}$ tuning/matching
knobs: yellow T & M



X tuning/matching
knobs: blue T & M